

750ml Ultrasonic Cleaning Equipment Portable CD Jewelry Fruits Mini 35W JP-900S

Our Product Introduction

for more products please visit us on skymenultrasonic.com

Basic Information

- Place of Origin: China
- Brand Name: skymen/OEM
- Certification: CE/FCC/RHoS
- Model Number: JP-900S
- Minimum Order Quantity: 1 unit
- Price: Negotiation
- Packaging Details: Colorful box / big Carton
- Delivery Time: In Stock
- Payment Terms: T/T, L/C, Paypal
- Supply Ability: 5000 units per month



Product Specification

- Model: JP-900S
- Tank Capacity: 750ml
- Tank Size: 150*130*50 Mm
- Unit Size: 200*175*145 Mm
- Packing Size: 240*200*200 Mm
- Certification: CE, RoHS, FCC ISO9001
- Power (W): 35W
- Ultrasonic Frequency: 42KHz
- Power Supply: AC 110V / AV220V
- G.W: 1.38kg
- Color: White
- Delivery: Immediately
- Origin: Guangdong, China (Mainland)
- Package Type: 1pcs/color Box, 6pcs/carton
- Timer: 5minutes Automatic OFF



More Images



Product Description

750ml Household Ultrasonic Bath

Pay attention: Don't start Ultrasonic cleaner before filling enough water in tank.

Application:

Jewelry, diamond, wedding ring, necklace, earring, body jewelry, body piercing, clock & watches, eyeglasses, contact lens, dentures, table-ware, printer inkjet, seal and comb, toothbrush, baby feeder, baby nipple, etc.and all your small things.

Specificatoin:

| | |
|------------------|--|
| Model | JP-900S |
| Tank capacity | 750ml |
| Ultrasonic power | 35W |
| Timer | 5 interval time adjustable |
| Frequency | 42,000Hz |
| N.W. | 0.95KG |
| Power Supply | AC 100 ~ 120V, 50 / 60Hz ; AC 220 ~ 240V, 50 / 60 Hz |
| Tank size | 150*130*50mm |
| Unit size | 200*175*145mm |
| Inner packing | 525*455*440mm |
| Carton packing | 545×510×355 mm |

Product description:

750ml digital ultrasonic cleaner, ultrasonic jewelry cleaning machine

JP-900S with 5 interval times settings

Having great effect of sterilizing and cleaning

Home used mini ultrasonic cleaner

Features

It presents the capacity of 750ml.

Ideal for cleaning spectacles, jewelry, dentures & Braces, cleaning watches and many more to maintain hygiene.

Presents a gentle cleaning method with a high cleaning frequency of 42KHz normally with a cleaning power of 35W.

Presents a stainless steel tank to use the cleaning fluid to clean the items at high frequency.

It vibrates at a high frequency to remove the dirt from the smallest and inaccessible particles.

Has a fine quality mesh basket for safe cleaning

Images of this model:



JP-900S more details:



1. Constructure


Sophisticated design for more elegant outlook.

2. Control panel design

5 digital timer settings: 90S, 180S, 280S, 380S, and 480S. Control panel is by whole conducting film slight touch design for more safe and leakproof.





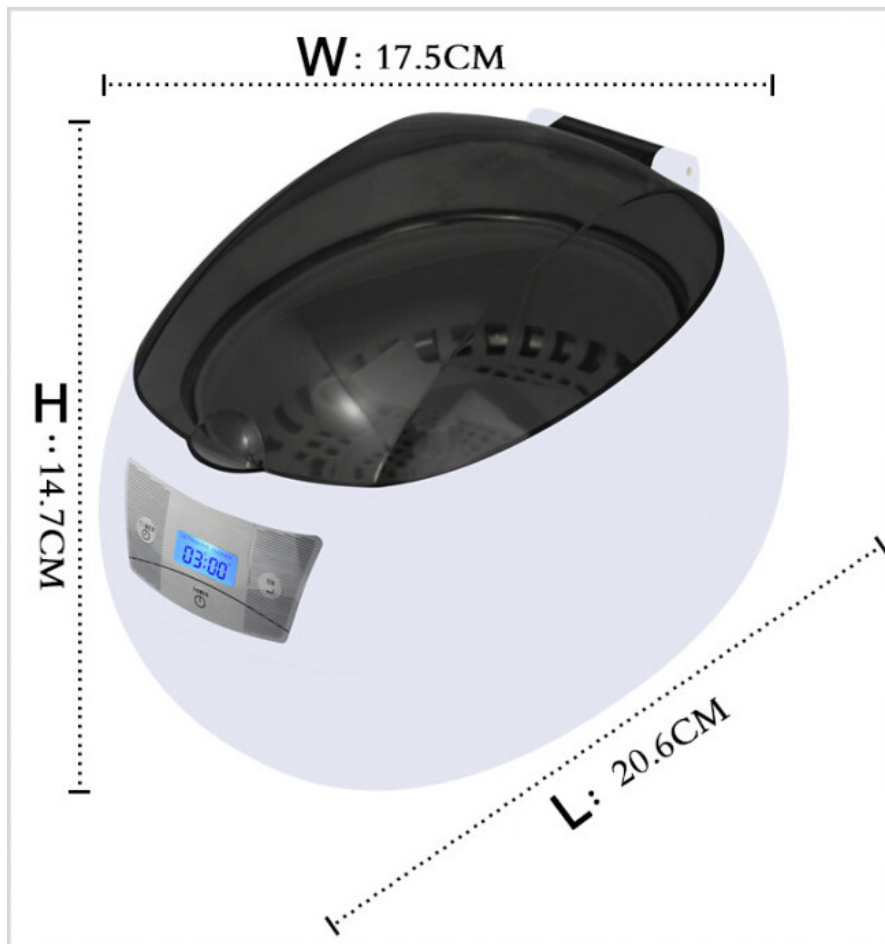


Clean pictures of this model:




How does Ultrasonic Cleaner work?

DIRT ELIMINATION PROCESS THROUGH ULTRASONIC TECHNOLOGY


- Cleaning effect will be much better if using the machine together with proper solvent.



As ultrasonic wave through the solution in the tank, cause alternating high and low pressures in the solution.



During the low pressure stage, millions of microscopic bubbles form and grow. This process is called "CAVITATION".



During the high pressure stage, the bubbles implode releasing enormous amounts of energy. They work in all directions, attacking surface and invading all recesses and openings.

How to use an ultrasonic cleaner? (take medical instruments as example)

In all cases manufacturers' instructions should be followed when using an ultrasonic cleaning process. These are representative steps.

Fill the ultrasonic cleaning tank with an approved medical instrument cleaning solution such as CLN-LR012 available from Tovatech following dilution instructions provided. Turn the cleaner on to start the degassing process. This step removes entrained air in new solutions that interferes with the efficiency of cavitation and takes approximately 10 minutes.

In the meantime:

Segregate instruments by alloy or composition to avoid potential damage (Chromium plated instruments should not be cleaned ultrasonically)

Instruments with movable parts should be disassembled to facilitate cleaning

Place the instruments the ultrasonic cleaner's mesh basket, taking care that they do not come in contact with each other
Cannulated or lumened instruments should be positioned to insure interiors are wetted with the cleaning solution. In some instances placing them on an angle will facilitate this

Set the control panel per manufacturers' instructions and start the cleaning process

At the end of the cycle, remove the instruments from the ultrasonic cleaning bath and thoroughly rinse them to remove all traces of the cleaning solution. Deionized water rinses will avoid spotting. If the instruments are not to be immediately disinfected and sterilized be certain that they are thoroughly dried and protected. Part reassembly can occur after sterilization. Procedures should be in place to guide the replacement of used ultrasonic cleaning solutions. In some instances it is recommended that solution be drained and tanks thoroughly cleaned and dried after each ultrasonic cleaning cycle. Most solutions available today are biodegradable, which facilitates disposal but local authorities should be consulted on proper practices.



Skymen Technology Corporation Limited



86-755-27094405



info@skymen.cc



skymenultrasonic.com

Floor 1st & 2nd, Building 3, Tanggang Taifeng Industrial Park, Dawangshan Community, Shajing Street, Bao'an District, Shenzhen